

WORK ORDER

CROWN BAR




1. Areas for implants

Please mark:


Implant Position

Biaxial Position X

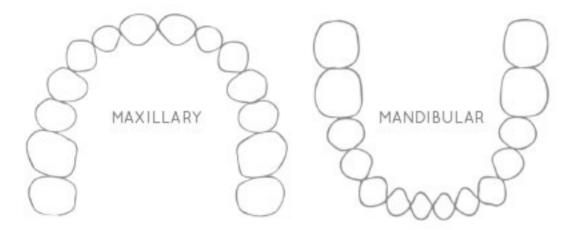

2. Design Instructions





Type B



Tissue Relationship Distance

As close as possible

Or specify____mm

Choose Material

Titanium

Co/Cr

ACCOUNT INFORMATION (please print)

Client Name						
Osteon Medical ACC#						
Bill to						
Ship to						
Contact						
Phone						
Email						
Patient ID						

3. Implant	System		

4. Date Required



5. Preparing Your Case For Shipment

IMPORTANT

- Only use new implant analogs
- Please do not send the articulator
- Please ensure analogs are proud of the stone model
- Minimum distance between implants is 2mm

PLEASE INCLUDE THE FOLLOWING:

- · Copy of completed work order
- Verified/Accurate soft tissue model
- · Resin pattern if copy mill bar is desired
- Verified denture set up (disinfected) with positive relationship to implant model

. Special	Requirements
-----------	--------------

200					
7.	Ce	rt	ifi	cat	ion

- I certify that the analogs are brand new and their positions have been verified for accuracy.
 All information stated on this work order is correct.
- . All items that have ontacted the oral environment have been disinfected.
- This work order authorizes Osteon Medical pty ltd to manufacture the
 Osteon structure using all relevant information provided on this work order.

Technician Signature ______ Date _____

CASE NUMBER # _____ Osteonmedical

